



390 TDS / Salt Meter

APPLICATIONS

Water:

Test TDS levels to determine purity

Food:

Test the amount of salt in food, seafood, or processed foods

Health:

Monitor the amount of salt intake

Water Filtration:

Test for TDS to determine performance level of filtration systems

Pools & Spas:

Monitor TDS levels to prevent maintenance problems

HVAC:

- Test condensate water in cooling tower and humidifier reservoir applications to prevent bacterial growth

- Test TDS levels in make-up water to prevent scale formation, corrosion, and embrittlement

- Reduce water and chemical consumption in boilers and cooling towers


- Determine when to perform blowdown and add make-up water

- Prevent contamination and corrosion of control valves, heat exchangers, and steam traps

- Verify automated TDS controllers are functioning properly

- Prevent low quality wet steam generation in boilers due to foaming caused by high TDS levels

Measure TDS (Total Dissolved Solid) and Salt Concentration

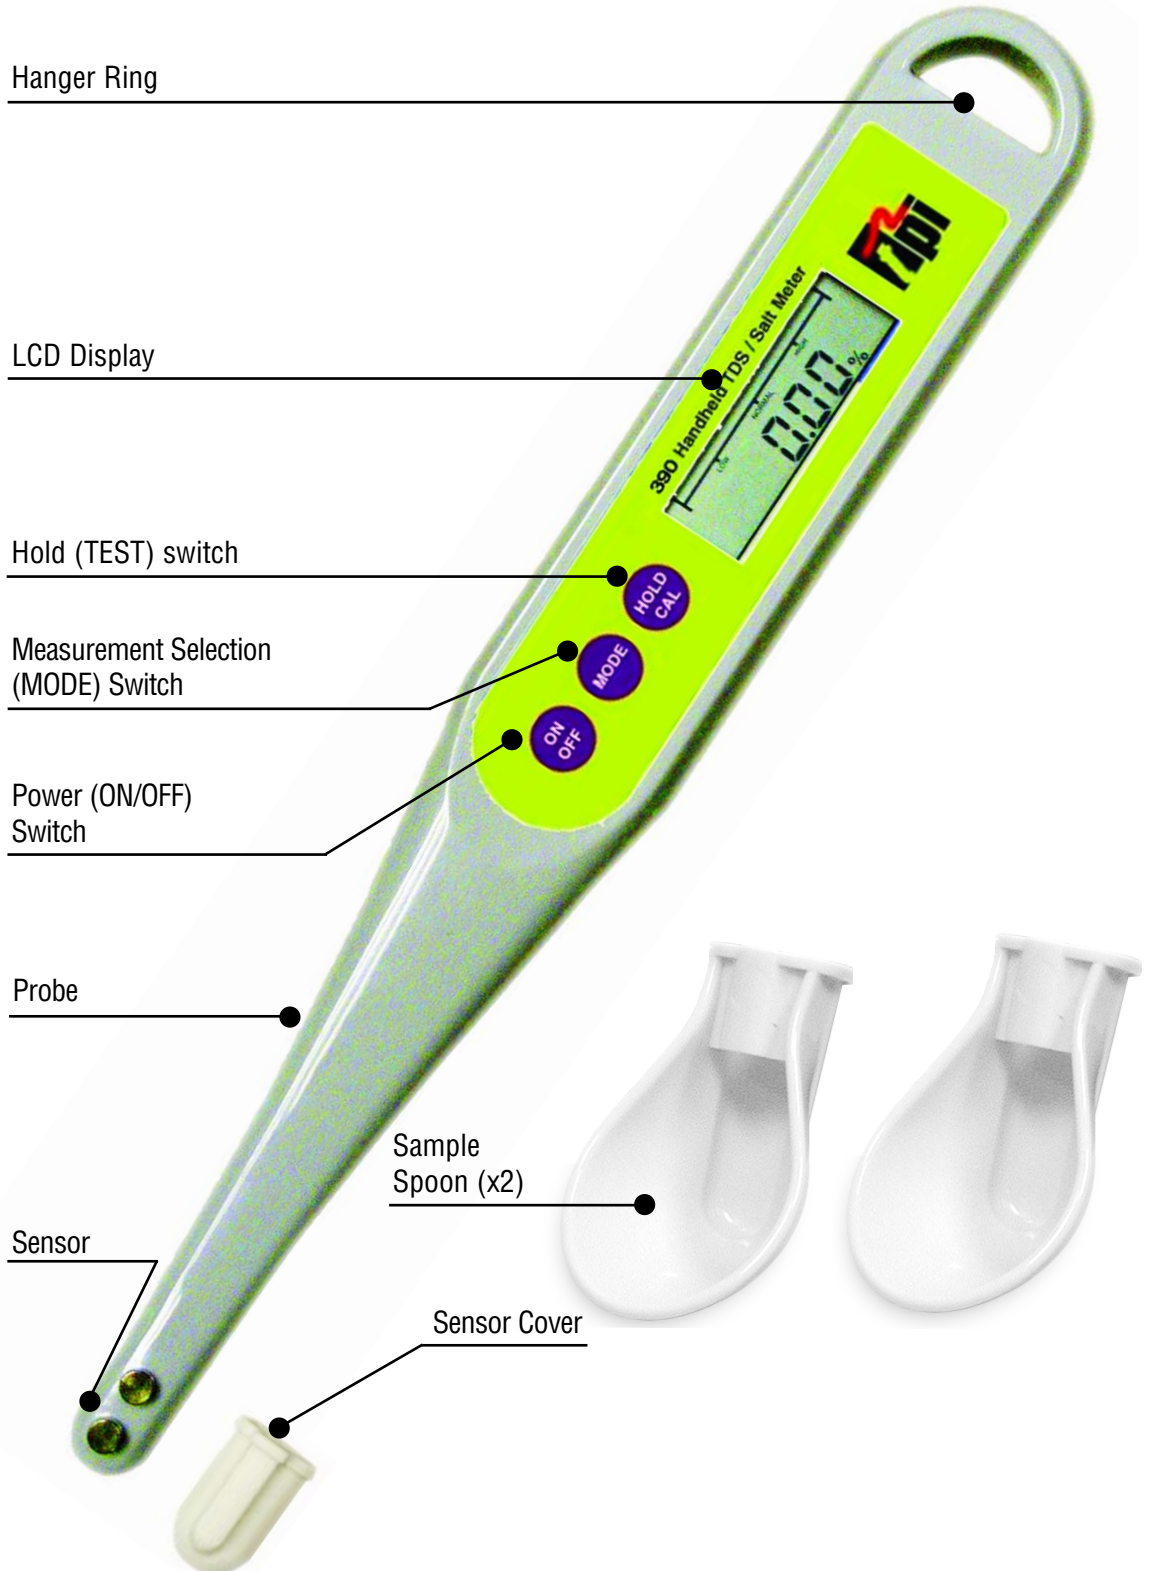

390 shown actual size: .63" x 1.26" x 10"



390 Specifications

TPI offers a complete line of...

CO, Combustibles & Combustion (CEA)

Refrigerant Leak Detectors

Digital Manometers

Temperature Contact & IR Instruments

IAQ: Air Flow & Humidity

Handheld Oscilloscopes

Digital Multimeters & Clamp-on Meters

Accessories & Kits

Test Products International, Inc.

Headquarters:
9615 SW Allen Blvd.
Beaverton, OR 97005
USA
503-520-9197
Fax: 503-520-1225
e-mail:
info@tpi-thevalueleader.com

Test Products International, Ltd.

342 Bronte St. South
Unit #9
Milton, Ontario L9T
5B7
Canada
905-693-8558
Fax: 905-693-0888
e-mail:
info@tpicanada.com

Test Products International UK Ltd.

Longley House,
East Park
Crawley, West Sussex
RH10 6AP England
Tel:
+44 (0)1293 561212
Fax:
+44 (0)1293813465
contactus@tpieurope.com

Measurement Target	Aqueous Solution
Salt Measurement	Measurement Method: Electric Conductivity Measurement System Measurement range: 0.001% to 5.0% Measurement Temp: 50°F to 104°F (10°C to 40°C) Measurement Temp. Range: 32°F to 158°F (0°C to 70°C)
Temperature Measurement	Measurement Range: 32°F to 212°F (0°C to 100°C) Measurement Accuracy: ±1°C (temp. range: 0°C to 70°C) of reading
TDS	Measurement Range: 0 to 999ppm (mg/L) Measurement Accuracy: ±3% full scale @ 20°C Excellent Temp. Range: 50°F to 86°F (10°C to 70°C) Measurement Temp. Range: 32°F to 104°F (0°C to 40°C)
Resolution @ 20°C	Salt Measurement: 0.01% to 0.1% TDS: 1ppm (mg/L)
Power Supply	LR44 or LR1154 Button Battery (x3)
Size	16.4mm x 32mm x 255mm
Standard Accessories	Sensor protection cap, supporting spoon (2), NaCl standard solution (40g), manual, and batteries

Distributed By:



To learn about the entire line of TPI products visit:

www.tpi-thevalueleader.com

FAQ

Why is controlling TDS levels important in HVAC applications?

High TDS levels in HVAC equipment cause corrosion, loss of efficiency, and premature failure.

What is the advantage of testing TDS in boiler applications?

By monitoring TDS levels in HVAC equipment, a proper blowdown schedule can be implemented to prevent premature failure and lower operating costs.

Why test drinking water for TDS?

The EPA advises the maximum contamination level (MCL) is 500ppm for TDS. TDS levels in excess of 1000ppm are generally considered unfit for human consumption. High levels of TDS warrant further investigation, as the cause may be toxic ions such as arsenic, cadmium, and nitrate.

How can TDS levels be reduced?

In drinking water, common ways to reduce TDS levels are, carbon water filters, reverse osmosis, and distillation.

What are acceptable levels of TDS in drinking water?

0 to 50ppm - Ideal drinking water usually attained through reverse osmosis, deionization, micro filtration, and distillation.

50 to 140ppm - Considered an acceptable level for carbon filtering.

140 to 400ppm - Average tap water

170ppm and above - Hard water

500ppm - EPA maximum contamination level.